

EndoPro **270**[™]

Cordless Powered Heat Source

Manufactured for



BRASSLER USA[®]
DENTAL INSTRUMENTATION

Operation & Maintenance Instruction Manual

PLEASE READ ALL INSTRUCTIONS PROVIDED FOR THIS DEVICE BEFORE USING IT.

Caution: This product should only be used by dental professionals after reading the instruction for use.

FULLY CHARGE BATTERY IMMEDIATELY UPON RECEIPT AND PRIOR TO FIRST USE.

Table of Contents

- 2 Introduction
- 2 Safety Instructions
- 2 Contraindications
- 2 Notes
- 3 Features
- 4 Product Description
- 5 How to Install/Change the Battery Pack
- 5 Attaching Pluggers to the Heating Unit
- 6 Caution During the Usage of this Device
- 7 Charging the Battery
- 8 Indications for Use
- 9 Troubleshooting
- 9 Sterilization & Maintenance
- 10 Warranty

CAUTIONS



This equipment conforms to the requirements of Medical Device Directive 93/42/EEC and satisfies the electrical safety requirements of EN 60601-1 and Electromagnetic emissions and immunity standards of EN 60601-1-2. These limits are designed to provide reasonable protection against harmful interference in a typical medical installation. However, because of the proliferation of radiofrequency transmitting equipment and other sources of electrical noise in healthcare environments (for example, electrosurgical units, cellular phones, mobile two-way radios, electrical appliances and high-definition television), it is possible that high levels of such interference due to close proximity or strength of a source, may result in disruption of performance of this device.

WARNING

Risk of Fire, Risk of Burning

Keep the heated tip away from skin and anything that is flammable.

Introductions

Thank you for purchasing the EndoPro270 device from Brasseler USA. This device is ideal for the safe and effective removal of root canal filling materials and supports obturation techniques that require warm vertical compaction of gutta-percha or Resilon® root canal filling materials. READ THIS MANUAL CAREFULLY AND BE FAMILIAR WITH ALL SAFETY PRECAUTIONS PRIOR TO USING THIS DEVICE.

Safety Instructions

- 1 Improper usage of this device may cause injury to patients, operators and dental assistants, and/or damage to the product.
- 2 It is intended exclusively for use by licensed dentists and endodontists only. Plugger Tips are very hot when device is activated, thus care must be taken by the dentist, assistant and patient not to contact the tip while hot. Usage of a rubber dam is strongly recommended for proper isolation of the tooth.
- 3 The temperature of the Plugger can reach 270°C, therefore, it should not be used inside the root canal for more than 5 seconds at a time.
- 4 Plugger Tips must be sterilized before first use and between patient uses. For sterilization of tip, temperature must not exceed more than 135°C in the autoclave.

Contraindications

- 1 Do not use any other Plugger Tips except the ones supplied by Brasseler USA. Use of any Plugger or battery that is not supplied by Brasseler USA may result in electrical shock, fire, or explosion and void Warranty.
- 2 Do not use the EndoPro270 device on patients with pacemakers.
- 3 Do not use the EndoPro270 device when the battery level displays red light. Charge the unit and wait for the device to display the green light.

Notes

- 1 It is recommended that battery be fully charged before using the EndoPro270 device for the first time. Allow approximately 3 hours for full charge.
- 2 The actual temperature of a EndoPro270 Plugger is within a range of +/- 40°C of the temperature displayed on the unit.

Features

EndoPro270 PACKAGE CONTENTS

- Heating Unit
- Charging Base
- Battery
- Adapter 12V, 1620mAH
- Power Cord
- Directions For Use
- Plugger (45/04)

Available Pluggers Include (Tip Size / Taper):

- SML(45/04)
- SML/MED(55/06)
- MED(55/08)
- MED/LRG(55/10)
- LRG(60/12)
- Spreader/T
- Thermal Tester

SPECIFICATIONS

Charging Base Dimensions: 81mm X 137mm X 36mm

Charging Base Weight: 207g

Heating Unit Dimensions: 12.5mm X 150.5mm X 21.5mm

Heating Unit Weight: 63g

TECHNICAL DATA

Battery: Li-Ion 3.7V


Source: 100~240V / 50~60Hz, DC 12V, 850mA

Operating Temperature: 0°C to 45°C, Storage Temperature: -20°C to 60°C

Product Description


HEATING UNIT

- ① Plugger
- ② Plugger Attachment Cap
- ③ Heater Switches
- ④ Battery Level Indicator
- ⑤ Temperature Display
- ⑥ Power "ON/OFF" Switch / Temperature Selection- Powers the unit on and off, and changes the temperature setting
- ⑦ Battery Casing

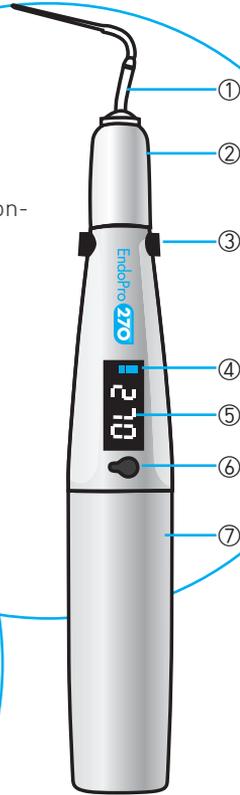


CHARGING BASE

- ① Charging Status Indicator
- ② Charging Contact Terminals

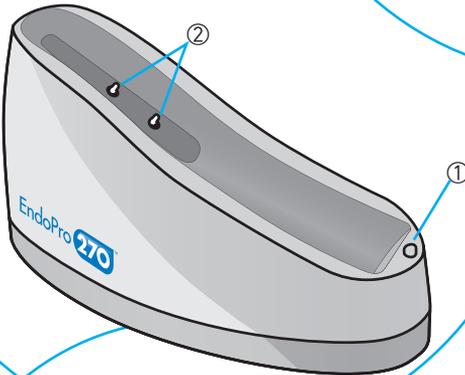

BATTERY

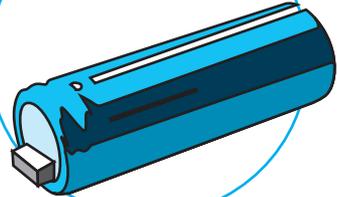


POWER ADAPTER



How to Install/Change the Battery Pack

- ① Insert the Battery Pack into the Heating Unit as shown in the pictures.
- ② Thread the Battery Casing onto the Heating Unit. Caution: Ensure threads are aligned and avoid excessive forces when threading the Battery Casing onto the Heating Unit.
- ③ When replacing the battery, turn the Battery Casing counterclockwise. Separate the Battery from the connector of the Heating Unit. See ① and ② above for installation instructions.

[Caution: When inserting the battery, make sure the connector is properly set].

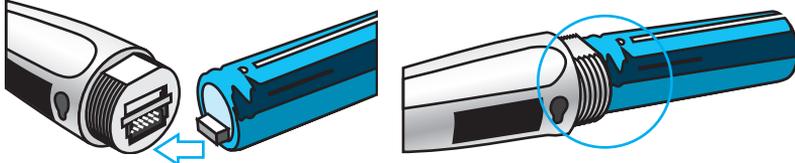

Attaching Pluggers to the Heating Unit

- ① Press the Power "ON/OFF" Switch button. If lights do not display, check the Battery connection. If the display window shows 'oPn', this indicates that the Plugger is not connected properly. When the Plugger is connected properly, the default temperature of 150°C or the last temperature setting will appear.
- ② To change the temperature setting, press the Power "ON/OFF" Switch until reaching the setting you desire. Pressing the switch will rotate temperature settings in the following order: 150°C → 180°C → 200°C → 230°C → 250°C → 270°C → 150°C.



Recommended Temperatures: EndoSequence®, ActivGP™ and Endo-Sequence® BC GuttaPercha - 230°C / Standard Gutta Percha - 200°C / Resilon® - 150°C / Carrier Handles - 270°C

Caution: Plugger is extremely hot during use. Avoid direct contact with the patient's soft tissue in the oral cavity.

Inserting Plugger



Note: The mouth of the Heating Unit has 6 different slots for inserting the Plugger. Select the appropriate one based on your preferred orientation of the Heater Switches in relation to the Plugger tip.

Heating the Plugger

Once the Plugger is properly connected to the Heating Unit, press the Power "ON/OFF" Switch to turn on the unit. When the power is on and the Plugger has been properly installed, the temperature will be displayed on the screen. Change the temperature if necessary.

Heating the Plugger occurs by pressing (and holding) either one of the two Heater Switches. Releasing the Heater Switch allows the Plugger to return to room temperature. During normal operation, a beeping noise will indicate that the Plugger is hot. Do not touch the Plugger until it has a chance to return to room temperature.

Caution During the Usage of this Device


- ① The EndoPro270 Heating Unit is designed to turn-off automatically if the battery should begin to overheat. While the chance of this occurring is rare, if it occurs, please allow the Heating Unit sufficient time to cool. Then, recharge the Heating Unit by placing it on the Charger Base for at least 30 seconds before attempting to use again.
- ② Heat activation of the Plugger inside the canal should not exceed more than 5 seconds.
- ③ This device shuts off automatically if not used for more than 10 minutes. Press the Power "ON/OFF" Switch to turn on the unit.
- ④ The tip of the Plugger is very hot during use. Please perform all endodontic procedures with a rubber dam.
- ⑤ For safety purposes, place the tip of the Plugger at the orifice of the root canal before activating the Heater Switches. Use caution to avoid contact to the soft tissue of the oral cavity while the Plugger is hot.
- ⑥ When replacing the Plugger, turn the power off and ensure the Plugger has cooled down sufficiently.
- ⑦ The Plugger should be sterilized prior to use. The Plugger can be sterilized in an autoclave in accordance with the sterilization guidelines of the autoclave's instruction manual.



NOTE: This device is only intended for use during root canal therapy. Use extreme caution with the Heating Unit so as not to burn the patient or oneself.

Charging the Battery

Keep the Heating Unit on the Charging Base while the unit is not in use. The Device is ready for use when the LED charging status indicator displays a green light. Once a red light on the Battery Indicator of the Heating Unit starts to flash, the unit needs to be recharged by carefully positioning the Heating Unit on the

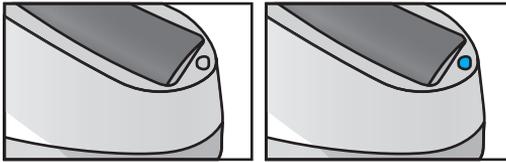


Charging (Amber)

Fully charged (Green)

Charging Base ensuring the proper contact is made. Once the battery is fully charged, the LED charging status indicator will turn green.


- ① Connect the Power Adapter to the Charging Base.
- ② Position the Heating Unit on the Charging Base correctly so that the Battery Charging Contact Terminals on the bottom of the Heating Unit align with the two Charging Contact Terminals on the Charging Base with the temperature display window facing upwards.
- ③ If the correct connection is made, the LED charging status will display an amber light during charging. Once the battery is fully charged, the LED charging status indicator will turn green.

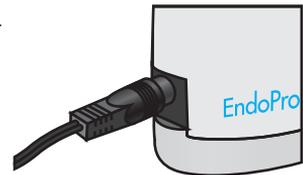

Note: If the LED is neither yellow or green, the charging terminals are not properly connected. Re-align the Heating Unit on the Charging Base and also check that you are getting power to the Charging Base.

Pluggers should be removed while charging. Please keep the pluggers disconnected from the unit after each treatment.

- ④ To confirm whether the battery is fully charged, separate the unit from the Charging Base and turn on the Heater Switch. If there are 3 levels of the green LED displayed, the unit is fully charged.



Note: If the unit has not been in use for more than a month, it may not function correctly due to natural discharge of the battery. Monthly recharging is recommended even when the unit has been fully charged but is not in use.

Indications for Use

- ① Sealing off Gutta-percha
- ② Post Preparations
- ③ Vitality testing (Heat test)
- ④ Warm vertical compaction
- ⑤ Warm lateral compaction



Note : Contact your Brasseler USA sales representative, if you have any technique questions retaining to the above indications for use.

Troubleshooting

Code	Description or possible causes	Recommended action for the user
Er0	Defective Microprocessor	If this error code is displayed on the screen please contact authorized dealer's customer service department.
oPn	This message will be displayed on the screen if the Plugger is not correctly connected to the unit and if the heating mechanism is not working properly.	Separate the Plugger from the unit and reconnect the Plugger. If proper temperature setting is displayed, it indicates normal state. If the same message is displayed, replace with a new Plugger and check to see if same problem occurs. If same problem occurs, please contact authorized dealer's customer service department.
SHR	Desired temperature not reached in 200 seconds: defective plugger or low battery power.	Recharge the battery or replace the plugger. If the code does not disappear, return the unit to authorized dealer for replacement.
HD1	Temperature does not change within 5 seconds after activation: Defective plugger. Power turns off while in use and power does not turn on again.	Replace the plugger. If the code does not disappear, return the unit to authorized dealer for replacement. A. This may result from the Device overheating. Let the unit cool and retry. B. Recharge. C. If the same problems occur after recharging, change the battery.

Sterilization & Maintenance

Keep this device at room temperature away from external shock or direct sunlight.

Heating Unit and Charging Base – Clean the exterior of the Heating Unit and Charging Base by using a soft cloth moistened with a mild detergent or rubbing alcohol. The surfaces should be sheathed with plastic barrier to prevent contamination and discoloration. The use of non-recommended cleaning agents could result in damage to the outer surface of the EndoPro 270 Device.

DO NOT use strong disinfectants or those that contain Bleach or Ammonium Chloride to clean the device.

DO NOT autoclave the Heating Unit or Charging Base.

Plugger – After each use, the Plugger should be sterilized by autoclave for 60 minutes at 121°C, 15 PSI. Dispose of used Plugger into a biohazard container.



Notice: If the unit is not used for an extended period of time (more than once per month), it may not work because of battery discharge. Periodical (once per month) recharge is recommended even if the Device is not used. It is recommended to change the battery every 6 months. Please contact authorized dealer to purchase a replacement battery.

Warranty

Brasseler USA warrants the EndoPro270 against defects in material and workmanship for 12 months from the date of purchase with proper usage. During that twelve-month period, Brasseler USA will repair or replace a defective unit. Defects caused by misuse, neglect, accident or abuse are not covered by this warranty. Brasseler USA assumes no liability resulting from improper use, damage or breakage due to misuse of the EndoPro270.

The manufacturer is not responsible for breakage of any component of the EndoPro270, including the Plugger, resulting from forceful compaction of gutta-percha or Resilon® or use of the Plugger outside of the indications noted in this Instruction for Use.

The battery and Pluggers in the EndoPro270 are replaceable. New batteries and Pluggers can be ordered from Brasseler USA.

Brasseler USA assumes no liability for damage to the EndoPro270, injuries to patients or users or other problems resulting from use of accessories or other materials not supplied by Brasseler USA.

For Sales Orders and Product Information Contact:

Brasseler USA
One Brasseler Blvd.
Savannah, GA 31419
800-841-4522
www.brasselerusa.com

Manufactured for



BRASSLER USA[®]
DENTAL INSTRUMENTATION